

AccuSpan™ HCV RNA Linearity Panel

2410-0327 / Batch #10343660


OVERVIEW

The AccuSpan™ HCV RNA Linearity Panel (2410-0327 / Batch #10343660) is an eight-member panel made from serial dilutions of high titer recombinant Hepatitis C virus (genotype 1b) with established reactivity for HCV RNA and one negative member. This panel consists of seven members representing serial log dilutions of AccuPlex recombinant HCV in negative diluent and one negative member prepared from the diluent. The diluent was prepared from pooled K3 EDTA plasma that was filtered through a 0.2 micron filter. Sodium azide (0.09%) was added as a preservative.

Results are reported for each panel member on specific test methods. Linearity is shown graphically by plotting observed results against expected results. The WHO International Standard was tested in the same run as the AccuSpan HCV RNA Linearity Panel members. Both expected and observed results for the standards are reported; expected results for the WHO standards are the WHO assigned values.

For Research Use Only. Not for use in diagnostic procedures. Data are provided for informational purposes. SeraCare Life Sciences does not claim that others can duplicate test results exactly.

CAUTION: Follow Universal Precautions.

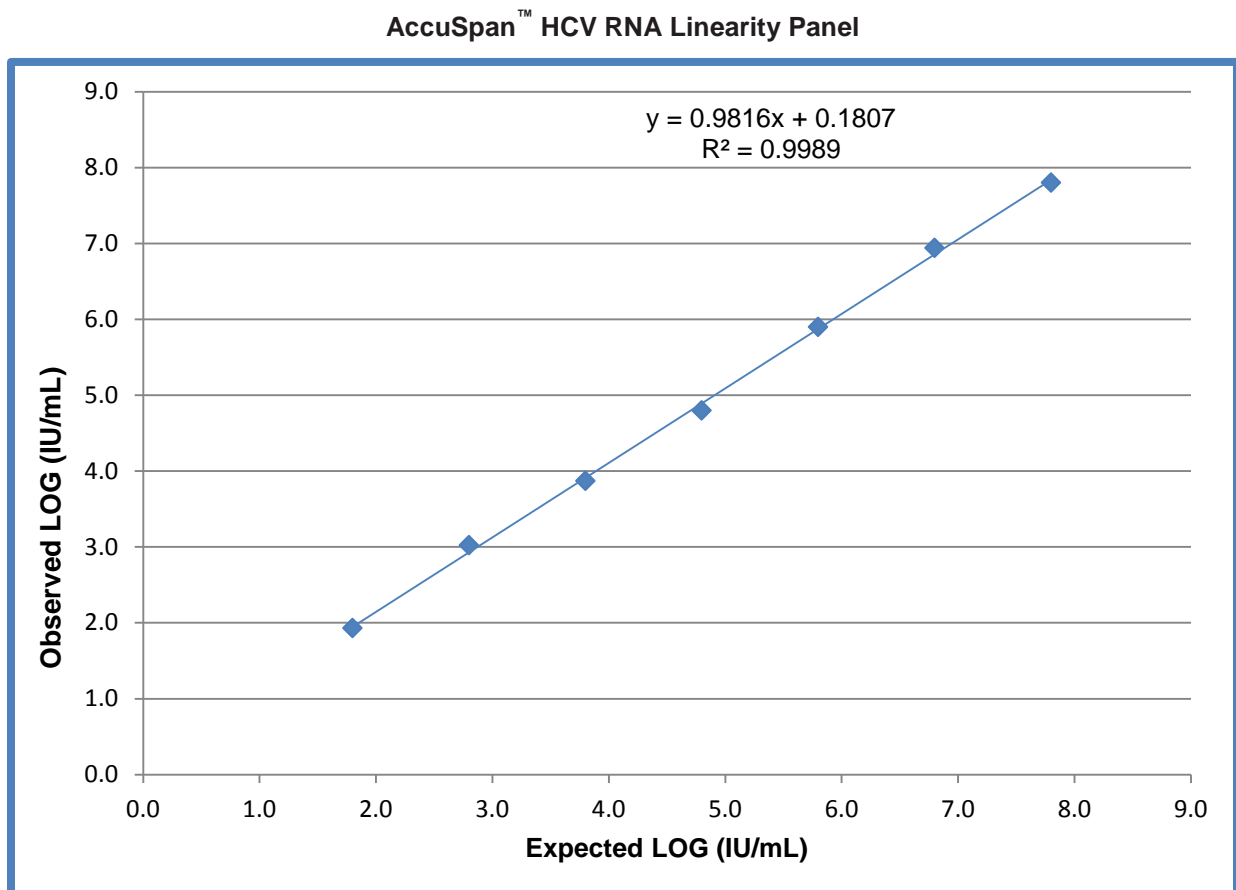

HCV RNA results were obtained using the Roche COBAS® AmpliPrep/COBAS® TaqMan® HCV Version 2.0 test method. Results are the mean of three replicates. A line of best fit is shown.

AccuSpan™ HCV RNA

Linearity Panel

2410-0327 / Batch #10343660

HCV RNA

Panel Member	Roche COBAS® AmpliPrep/COBAS® TaqMan® HCV Version 2.0 ^{1,2} (log IU/mL)	Abbott m2000 RealTime HCV ^{1,2} (log IU/mL)
01	7.80 ³	7.47
02	6.94	6.48
03	5.90	5.50
04	4.80	4.52
05	3.87	3.51
06	3.02	2.55
07	1.93	1.72
08	TND	TND
Test Date	16-May-2018 31-May-2018 ³ 01-Jun-2018 ³	07-May-2018
Test Site	RL	RL
Test Kit Range	15 to 100,000,000 IU/mL 1.18 to 8.00 log IU/mL	12 to 100,000,000 IU/mL 1.08 to 8.00 log IU/mL
Test Kit Part Code	NA	NA
Test Kit Lot No.	Y2328700000	480647
Test Kit Regulatory Status	IVD/CE	IVD/CE

¹Results are reported as log international units per mL (log IU/mL); positive/reactive results are noted in bold red.

²Results are reported as the mean result of triplicate testing.

³Panel Member #1 was tested at a 1:100 dilution and results were corrected for dilution factor. Testing was performed on 31-May-2018 and 01-Jun-2018.

TND = Target Not Detected; RL = Reference Lab; NA = Not available
IVD = In Vitro Diagnostic; CE = Conformité Européenne or CE Marking

AccuSpan™ HCV RNA Linearity Panel

2410-0327 / Batch #10343660

4th WHO International HCV RNA Standard (06/102)

Sample ID	Expected Values (log IU/mL)	Observed Values on Roche COBAS® AmpliPrep/COBAS® TaqMan® HCV Version 2.0	
		(log IU/mL) ¹	% Difference ²
Sample 1	4.70	4.37	-7.08
Sample 2	4.00	3.77	-5.77
Sample 3	3.70	3.50	-5.33
Sample 4	3.00	3.05	1.68
Test Date		16-May-2018	
Test Site		RL	
Test Kit Range		15 to 100,000,000 IU/mL 1.18 to 8.00 log IU/mL	
Kit Part Code		NA	
Kit Lot No.		Y2328700000	
Kit Regulatory Status		IVD/CE	

¹WHO panel was tested in the same test run as the AccuSpan™ HCV RNA Linearity Panel members. Samples were run in singlet. Positive/reactive results are noted in bold red.

²Percentage difference is how much the observed concentration differs from the expected concentration. Values calculated for reference only. Laboratories may use the data to apply a correction factor to the test results.

RL = Reference Lab; NA = Not available

IVD = In Vitro Diagnostic; CE = Conformité Européenne or CE Marking